



Pg(Progesterone) ELISA Kit

Cat# E0119

store at -20°C and 4°C for 6 months

INFORMATION

Size	96T
Applications	ELISA
Sensitivity	0.15ng/mL
Detection Range	0.31-20ng/mL
Specificity	This kit recognizes Pg in samples. No significant cross-reactivity or interference between Pg and analogues was observed.
Repeatability	Coefficient of variation is <10%
Background	<p>Progesterone belongs to a group of steroid hormones called progestogens. It is mainly secreted by the corpus luteum in the ovary during the second half of the menstrual cycle. It plays important roles in the menstrual cycle and in maintaining the early stages of pregnancy. During the menstrual cycle, when an egg is released from the ovary at ovulation, the remnants of the ovarian follicle that enclosed the developing egg form a structure called the corpus luteum [1]. This releases progesterone and, to a lesser extent, oestradiol. The progesterone prepares the body for pregnancy in the event that the released egg is fertilized. If the egg is not fertilized, the corpus luteum breaks down, the production of progesterone falls and a new menstrual cycle begins. Once the placenta develops, it also begins to secrete progesterone, supporting the corpus luteum. This causes the levels to remain elevated throughout the pregnancy, so the body does not produce more eggs. It also helps prepare the breasts for milk production. Uses of progesterone include hormone replacement therapy, birth control, support of fertility and pregnancy (e.g., prevention of preterm birth and miscarriage), and treatment of gynecological conditions.</p> <p>1. Blakemore,C. and S. Jennett. 2001. The Oxford Companion to the Body. New York: Oxford University. 2. Matijevic R, Grgic O. Predictive values of ultrasound monitoring of the menstrual cycle. Curr Opin Obstet Gynecol. 2005 , 17(4): 405 4103. Young JR, Jaffe RB. Strength duration characteristics of est rogen effects on gonadotropin response to gonadotropin releasing hormone in women.</p>

Test principle	This ELISA kit uses the Competitive-ELISA principle. The micro ELISA plate provided in this kit has been pre-coated with Pg. During the reaction, Pg in the sample or standard competes with a fixed amount of Pg on the solid phase supporter for sites on the Biotinylated Detection Ab specific to Pg. Excess conjugate and unbound sample or standard are washed from the plate, and Avidin conjugated to Horseradish Peroxidase (HRP) are added to each microplate well and incubated. Then a TMB substrate solution is added to each well. The enzyme-substrate reaction is terminated by the addition of stop solution and the color change is measured spectrophotometrically at a wavelength of 450 nm ± 2 nm. The concentration of Pg in the samples is then determined by comparing the OD of the samples to the standard curve.
----------------	---

Kit components & Storage

Item	Specifications	Storage
Micro ELISA Plate (Dismountable)	8 wells ×12 strips	-20°C, 6 months
Reference Standard	2 vials	
Concentrated Biotinylated Detection Ab (100×)	1 vial, 120 uL	
Concentrated HRP Conjugate (100×)	1 vial, 120 μL	-20°C(shading light), 6 months
Reference Standard & Sample Diluent	1 vial, 20 mL	4°C, 6 months
Biotinylated Detection Ab Diluent	1 vial, 14 mL	
HRP Conjugate Diluent	1 vial, 14 mL	
Concentrated Wash Buffer (25×)	1 vial, 30 mL	
Substrate Reagent	1 vial, 10 mL	4°C(shading light)
Stop Solution	1 vial, 10 mL	4°C
Plate Sealer	5 pieces	
Product Description	1 copy	
Certificate of Analysis	1 copy	

Note: All reagent bottle caps must be tightened to prevent evaporation and microbial pollution. The volume of reagents in partial shipments is a little more than the volume marked on the label, please use accurate measuring equipment instead of directly pouring.

Other supplies required

- Microplate reader with 450 nm wavelength filter
- High-precision transfer pipette, EP tubes and disposable pipette tips
- 37°C Incubator
- Deionized or distilled water
- Absorbent paper
- Loading slot for Wash Buffer

Note

1. Please wear lab coats, eye protection and latex gloves for protection. Please perform the experiment following the national security protocols of biological laboratories, especially when detecting blood samples or other bodily fluids.

2. A freshly opened ELISA Plate may appear to have a water-like substance, which is normal and will not have any impact on the experimental results.

3. Do not reuse the diluted standard, biotinylated detection Ab working solution, concentrated HRP conjugate working solution. The unspent undiluted concentrated biotinylated detection Ab (100×) and other stock solutions should be stored according to the storage conditions in the above table.

4. The microplate reader should be able to be installed with a filter that can detect the wave length at 450 ± 10 nm. The optical density should be within 0~3.5.

5. Do not mix or use components from other lots.

6. Change pipette tips in between adding of each standard level, between sample adding and between reagent adding. Also, use separate reservoirs for each reagent.

Sample collection

Serum: Allow samples to clot for 2 hours at room temperature or overnight at 4°C before centrifugation for 20 min at 1000×g at 2-8°C. Collect the supernatant to carry out the assay. Blood collection tubes should be disposable and be non-endotoxin.

Plasma: Collect plasma using EDTA-Na₂ as anticoagulant. Centrifuge samples for 15 min at 1000×g at 2-8°C within 30 min of collection. Collect the supernatant to carry out the assay. Hemolysed samples are not suitable for ELISA assay!

Urine: Use a sterile container to collect urine samples. Remove particulates by centrifugation for 15 minutes at 1000×g at 2-8°C. Collect the supernatant to carry out the assay.

Saliva: Remove particulates by centrifugation for 10 minutes at 4000×g at 2-8°C. Collect the supernatant to carry out the assay. Recommend to use fresh saliva samples.


Note for sample

1. Samples should be assayed within 7 days when stored at 4°C, otherwise samples must be divided up and stored at -20°C (≤1 month) or -80°C (≤3 months). Avoid repeated freeze-thaw cycles.
2. Please predict the concentration before assaying. If the sample concentration is not within the range of the standard curve, users must determine the optimal sample dilutions for their particular experiments.
3. It is recommended to do the experiment with undiluted human serum, plasma and saliva samples, urine samples diluted at about 10 fold.
4. It is recommended to do the experiment with undiluted serum and plasma samples from mouse, rat, chicken, porcine, bovine and sheep.

Reagent preparation

1. Bring all reagents to room temperature (18~25°C) before use. Follow the Microplate reader manual for set-up and preheat it for 15 min before OD measurement.
2. Wash Buffer: Dilute 30 mL of Concentrated Wash Buffer with 720 mL of deionized or distilled water to prepare 750 mL of Wash Buffer. Note: if crystals have formed in the concentrate, warm it in a 40°C water bath and mix it gently until the crystals have completely dissolved.
3. Standard working solution: Centrifuge the standard at 10,000×g for 1min. Add 1.0mL of Reference Standard & Sample Diluent, let it stand for 10min and invert it gently several times. After it dissolves fully, mix it thoroughly with a pipette. This reconstitution produces a working solution of 20 ng/mL. Then make serial dilutions as needed. The recommended dilution gradient is as follows: 20, 10, 5, 2.5, 1.25, 0.62, 0.31, 0 ng/mL.

Dilution method: Take 7 EP tubes, add 500uL of Reference Standard & Sample Diluent to each tube. Pipette 500uL of the 20 ng/mL working solution to the first tube and mix up to produce a 10 ng/mL working solution. Pipette 500uL of the solution from the former tube to the latter one according to this step. The illustration below is for reference. Note: the last tube is regarded as a blank. Don't pipette solution into it from the former tube.

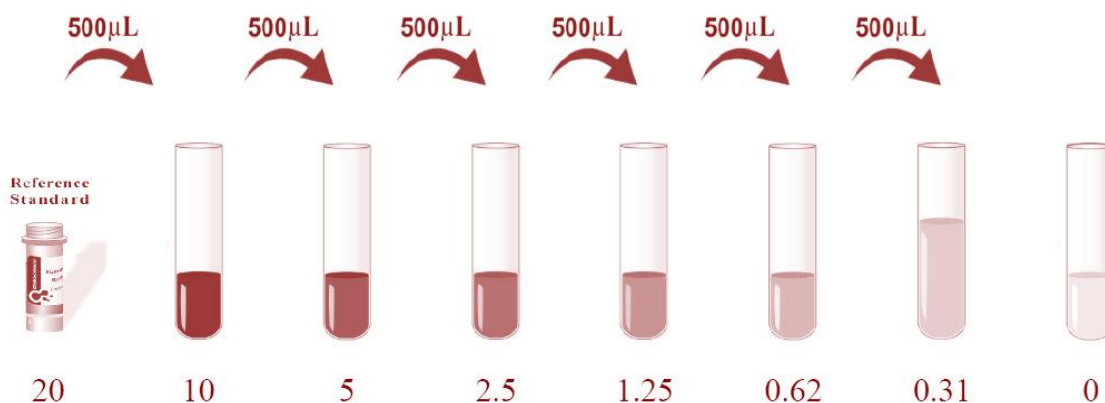

4. Biotinylated Detection Ab working solution: Calculate the required amount before the experiment (50 μ L/well). In preparation, slightly more than calculated should be prepared. Centrifuge the stock tube before use, dilute the 100 \times Concentrated Biotinylated Detection Ab to 1 \times working solution with Biotinylated Detection Ab Diluent.

5. Concentrated HRP Conjugate working solution: Calculate the required amount before the experiment (100 μ L/well). In preparation, slightly more than calculated should be prepared. Centrifuge the stock tube before use, dilute the 100 \times Concentrated HRP Conjugate to 1 \times working solution with Concentrated HRP Conjugate Diluent.

Assay procedure

1. Add the Standard working solution to the first two columns: Each concentration of the solution is added in duplicate, to one well each, side by side(50 μ L for each well). Add the samples to the other wells(50 μ L for each well). Immediately add 50 μ L of Biotinylated Detection Ab working solution to each well. Cover the plate with the sealer provided in the kit. Incubate for 45 min at 37 $^{\circ}$ C. Note: solutions should be added to the bottom of the micro ELISA plate well, avoid touching the inside wall and causing foaming as much as possible.

2. Aspirate or decant the solution from each well, add 350 μ L of wash buffer to each well. Soak for 1~2 min and aspirate or decant the solution from each well and pat it dry against clean absorbent paper. Repeat this wash step 3 times. Note: a microplate washer can be used in this step and other wash steps.

3. Add 100 μ L of HRP Conjugate working solution to each well. Cover with the Plate sealer. Incubate for 30 min at 37 $^{\circ}$ C.

4. Aspirate or decant the solution from each well, repeat the wash process for five times as conducted in step 2.

5. Add 90 μ L of Substrate Reagent to each well. Cover with a new plate sealer. Incubate for about 15 min at 37 $^{\circ}$ C. Protect the plate from light. Note: the reaction time can be shortened or extended according to the actual color change, but not more than 30min.

6. Add 50 μ L of Stop Solution to each well. Note: Adding the stop solution should be done in the same order as the substrate solution.

7. Determine the optical density (OD value) of each well at once with a micro-plate reader set to 450 nm.

Calculation of results


Average the duplicate readings for each standard and samples. Plot a four-parameter logistic curve on log-log graph paper, with standard concentration on the x-axis and OD values on the y-axis.

If the samples have been diluted, the concentration calculated from the standard curve must be multiplied by the dilution factor. If the OD of the sample is under the lowest limit of the standard curve, you should re-test it with an appropriate dilution. The actual concentration is the calculated concentration multiplied by the dilution factor.

Typical data

As the OD values of the standard curve may vary according to the conditions of the actual assay performance (e.g. operator, pipetting technique, washing technique or temperature effects), the operator should establish a standard curve for each test. Typical standard curve and data is provided below for reference only.

Concentration(ng/mL)	20	10	5	2.5	1.25	0.62	0.31	0
OD	0.091	0.142	0.315	0.642	0.917	1.460	2.144	2.898

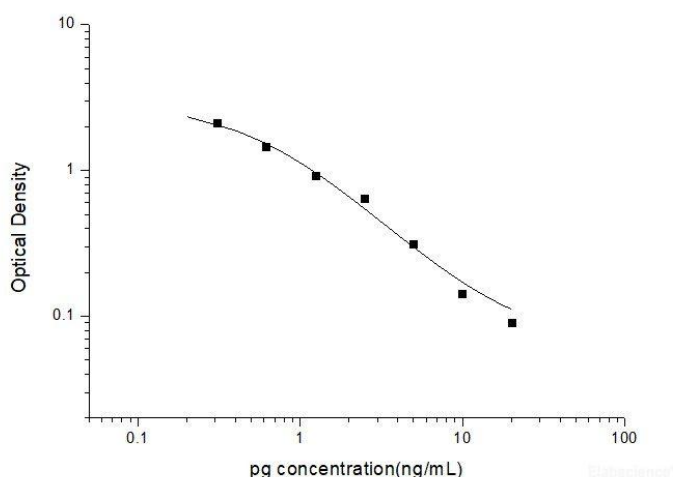

Reference values

Samples from different species were evaluated for the presence of Pg in this assay.

Sample type	Reference range of Pg in different species(ng/mL)						
	Human	Female Rat	Female Mouse	Chicken	Porcine	Sheep	Bovine
Serum(n=10)	0.52-3.09	4.1-8.2	0.-0.65	1.71-3.06	0.94-2.59	0.56-2.8	0.88-3.97
Plasma(EDTA)(n=10)	0.42-2.42	4.5-4.8	0-0.59	1.7-2.0	0.61-1.72	0.50-3.4	0.49-2.54
Urine(n=10)	8.39-117	-	-	-	-	-	-
Saliva(n=5)	0.7-1.97	-	-	-	-	-	-

The above values were all from normal healthy samples during non-physiological period or pregnancy.

Precision

Intra-assay Precision (Precision within an assay): 3 human samples with low, mid range and high level Pg were tested 20 times on one plate, respectively.

Inter-assay Precision (Precision between assays): 3 human samples with low, mid range and high level Pg were tested on 3 different plates, 20 replicates in each plate.

Sample	Intra-assay Precision			Inter-assay Precision		
	1	2	3	1	2	3
n	20	20	20	20	20	20
Mean(ng/mL)	0.56	2.22	8.78	0.54	2.01	8.55
Standard deviation	0.05	0.14	0.53	0.05	0.14	0.53
CV(%)	8.39	6.42	5.98	9.35	7.04	6.21

Recovery

The recovery of Pg spiked at three different levels in human samples throughout the range of the assay was evaluated in various matrices.

Sample Type	Range (%)	Average Recovery (%)
Serum(n=5)	80-94	84
EDTA plasma(n=5)	82-96	87
Urine(n=5)	85-109	95

Linearity

Human samples were spiked with high concentrations of Pg and diluted with Reference Standard & Sample Diluent to produce samples with values within the range of the assay.

		Serum(n=5)	Plasma (EDTA)(n=5)	Urine (n=5)
1:2	Range (%)	83-90	83-102	84-108
	Average (%)	85	90	93
1:4	Range (%)	80-95	82-95	80-112
	Average (%)	89	89	92
1:8	Range (%)	89-100	81-89	86-96
	Average (%)	92	86	87
1:16	Range (%)	87-102	87-115	84-94
	Average (%)	91	98	88

Troubleshooting


Problem	Causes	Solutions
Poor standard curve	Inaccurate pipetting	Check pipettes.
	Improper standard dilution	Ensure briefly spin the vial of standard and dissolve the powder thoroughly by gentle mixing.
	Wells are not completely aspirated	Completely aspirate wells in between steps.
Low signal	Insufficient incubation time	Ensure sufficient incubation time.
	Incorrect assay temperature	Use recommended incubation temperature. Bring substrate to room temperature before use.
	Inadequate reagent volumes	Check pipettes and ensure correct preparation.
	Improper dilution	
HRP conjugate inactive or TMB failure	Mix HRP conjugate and TMB, rapid coloring.	
Deep color but low value	Plate reader setting is not optimal	Verify the wavelength and filter setting on the Microplate reader.
		Open the Microplate Reader ahead to pre-heat.
Large CV	Inaccurate pipetting	Check pipettes.
High background	Concentration of target protein is too high	Use recommended dilution factor.
	Plate is insufficiently washed	Review the manual for proper wash. If using a plate washer, check that all ports are unobstructed.
	Contaminated wash buffer	Prepare fresh wash buffer.
Low sensitivity	Improper storage of the ELISA kit	All the reagents should be stored according to the instructions.
	Stop solution is not added	Stop solution should be added to each well before measurement.

SUMMARY

1. Add 50 μ L standard or sample to each well. Immediately add 50 μ L Biotinylated Detection Ab to each well. Incubate for 45 min at 37°C
2. Aspirate and wash 3 times
3. Add 100 μ L HRP Conjugate to each well. Incubate for 30 min at 37°C
4. Aspirate and wash 5 times
5. Add 90 μ L Substrate Reagent. Incubate 15 min at 37°C
6. Add 50 μ L Stop Solution. Read at 450nm immediately.
7. Calculation of results.

Declaration

1. Limited by current conditions and scientific technology, we can't conduct comprehensive identification and analysis on all the raw material provided. So there might be some qualitative and technical risks for users using the kit.
2. The final experimental results will be closely related to the validity of products, operational skills of the operators and the experimental environments. Please make sure that sufficient samples are available.
3. To get the best results, please only use the reagents supplied by the manufacturer and strictly comply with the instructions!
4. Incorrect results may occur because of incorrect operations during the reagents preparation and loading, as well as incorrect parameter settings of the Micro-plate reader. Please read the instructions carefully and adjust the instrument prior to the experiment.
5. Even the same operator might get different results in two separate experiments. In order to get reproducible results, the operation of every step in the assay should be controlled.
6. Every kit has strictly passed QC test. However, results from end users might be inconsistent with our data due to some variables such as transportation conditions, different lab equipments, and so on. Intra-assay variance among kits from different batches might arise from the above reasons, too.

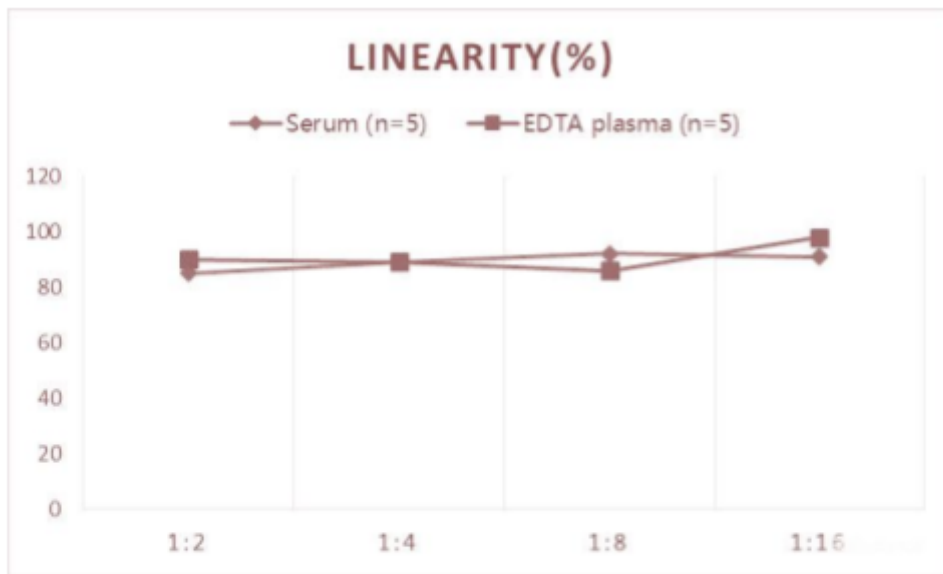

PRODUCT USE LIMITATION

These products are intended for research use only